

FIG. 1

Prediction Error for *In Vivo* Measurement of Blood Glucose Concentration

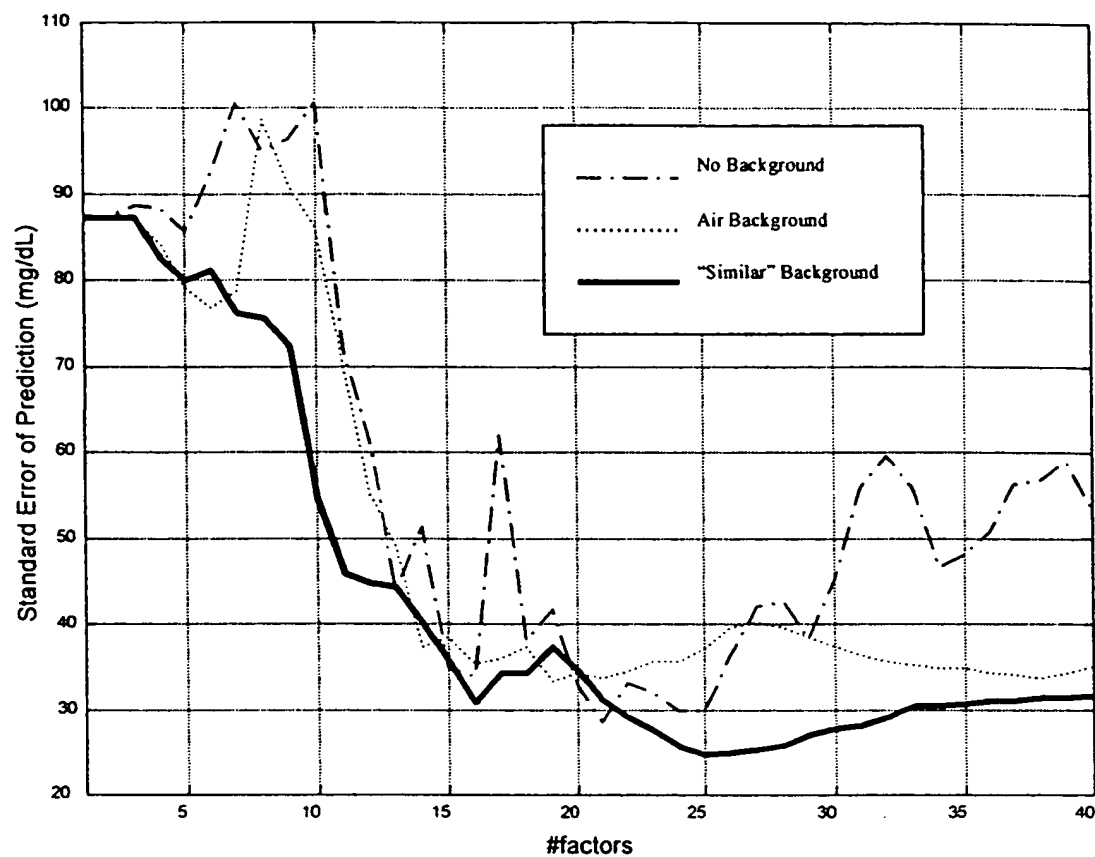


FIG. 2

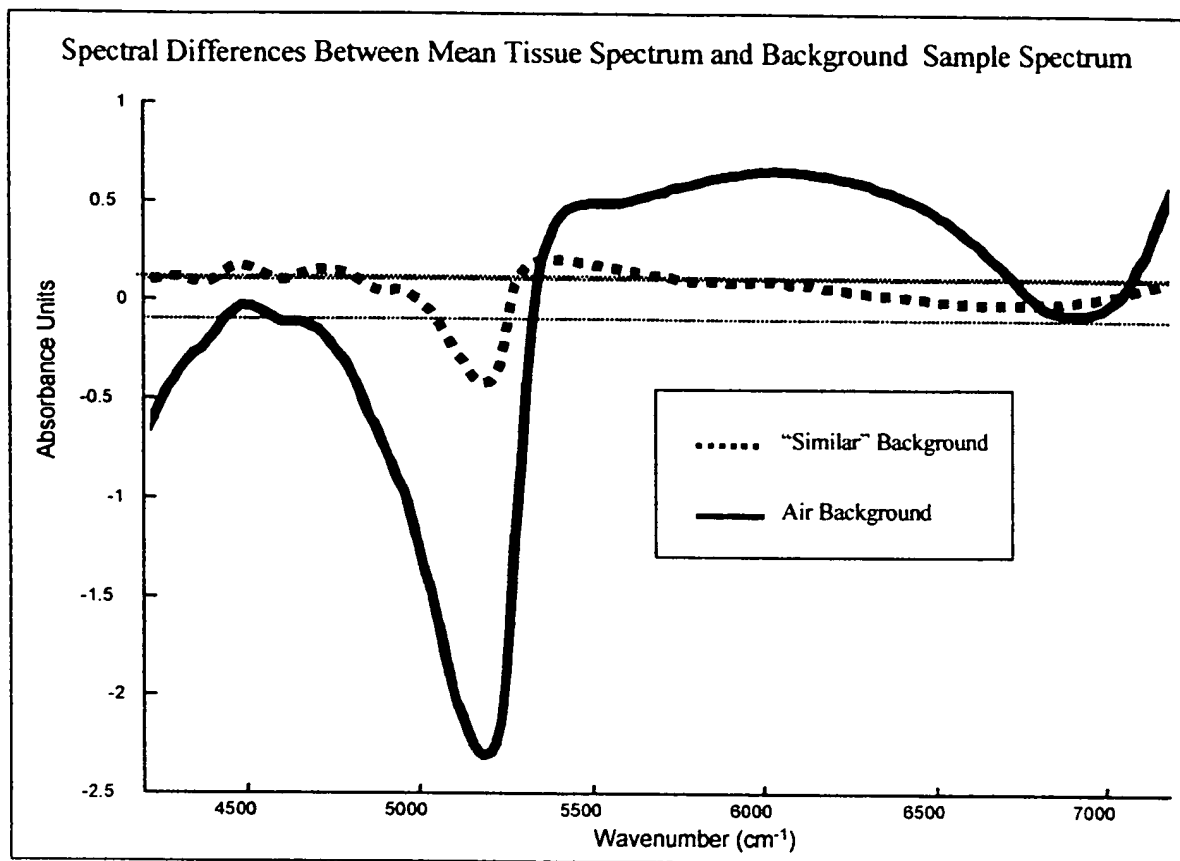


FIG. 3

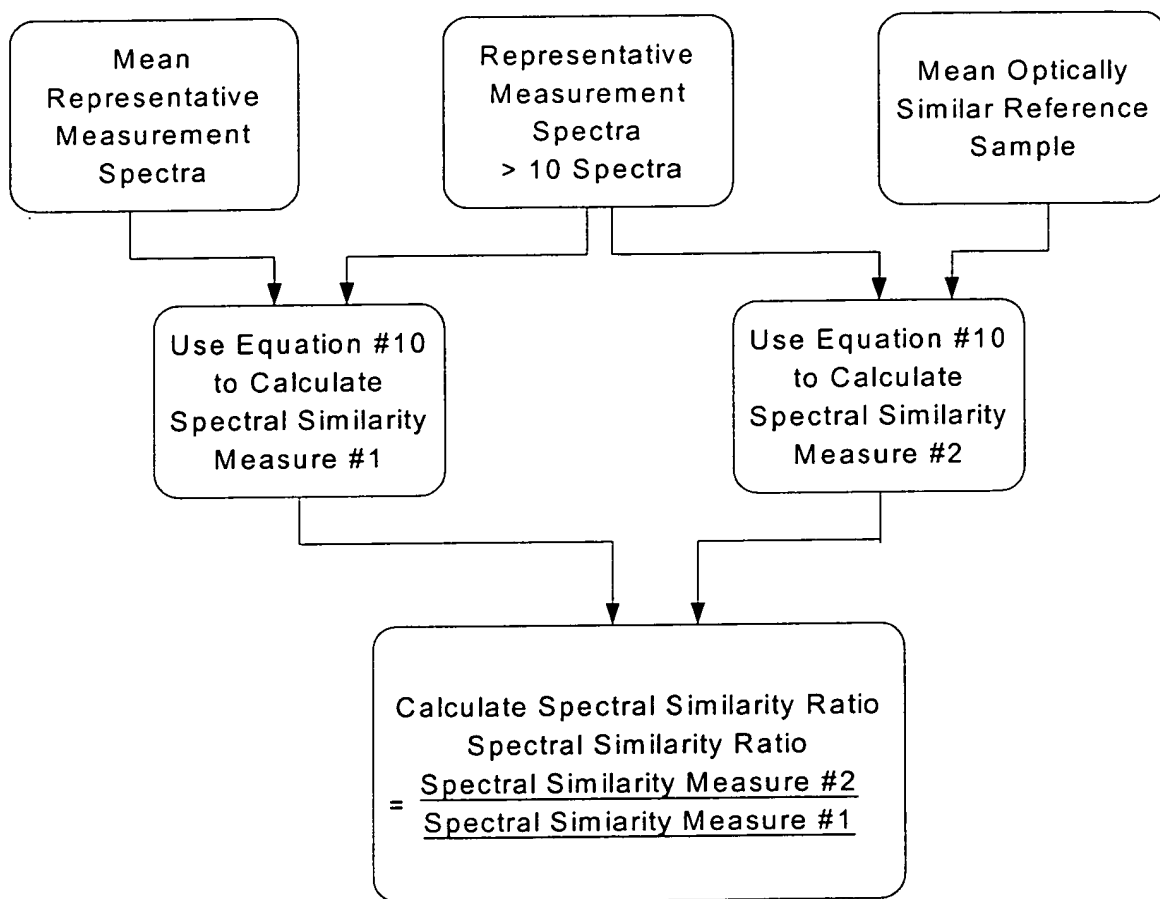


FIG 4

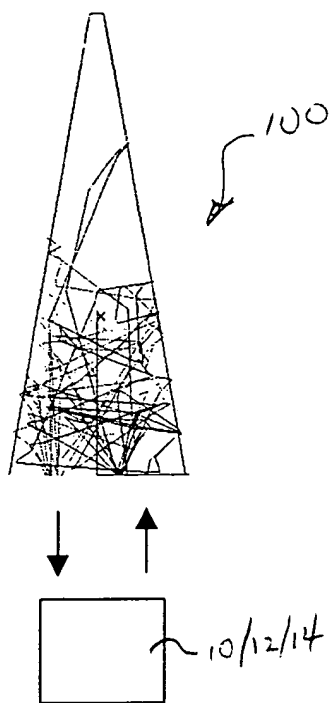


FIG. 5

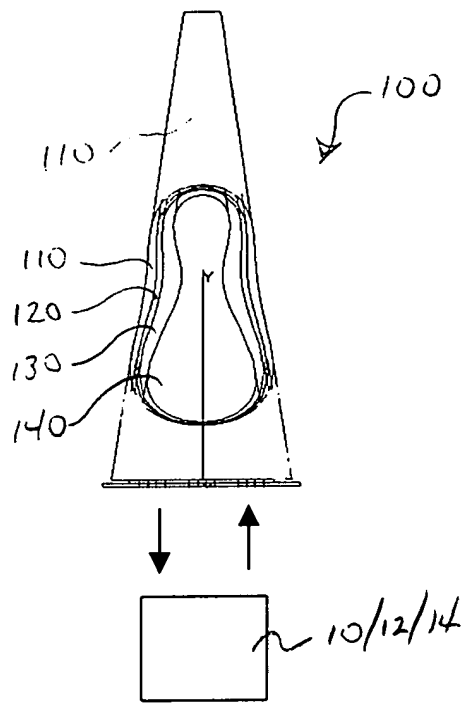


FIG. 6

AU

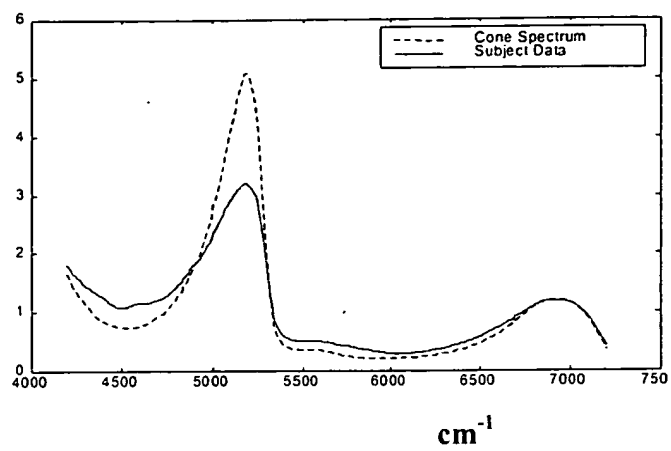


FIG 7

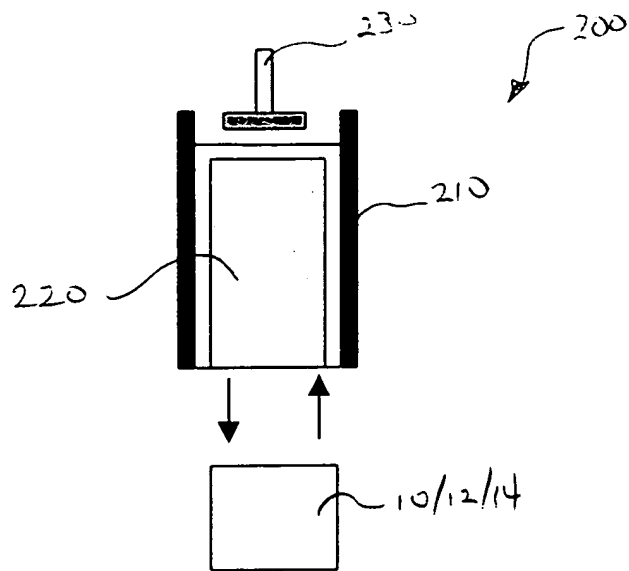


FIG. 8

FIG. 9

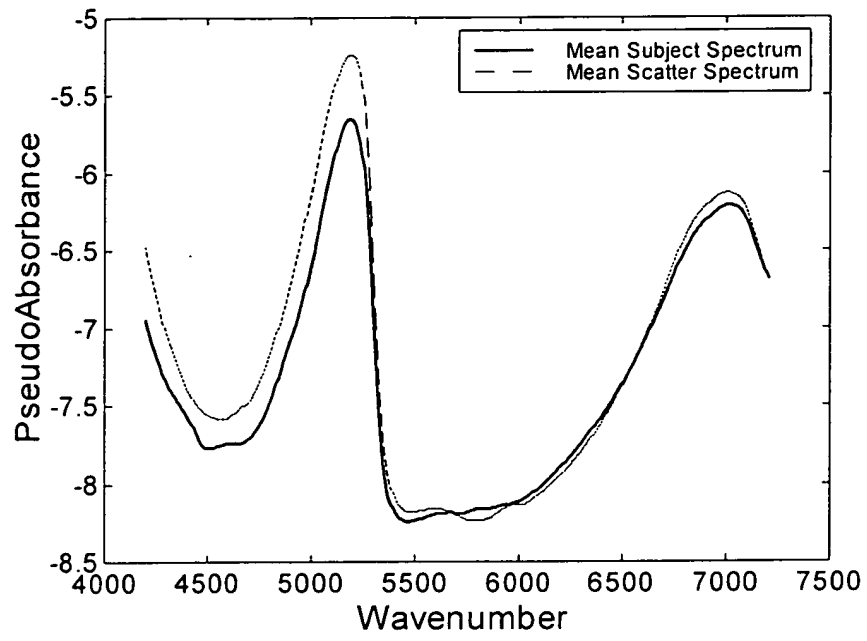


FIG. 9

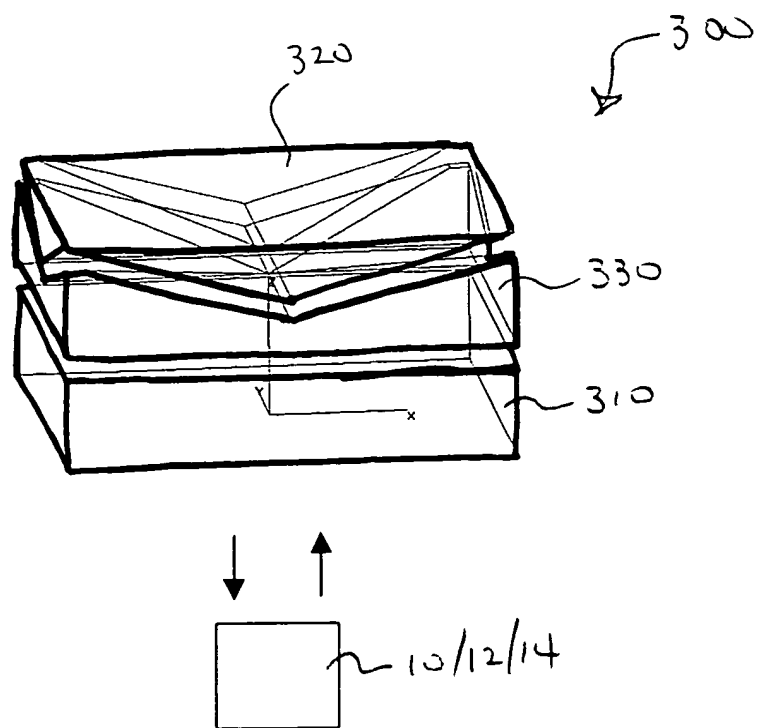


FIG. 10A

0922600-04101

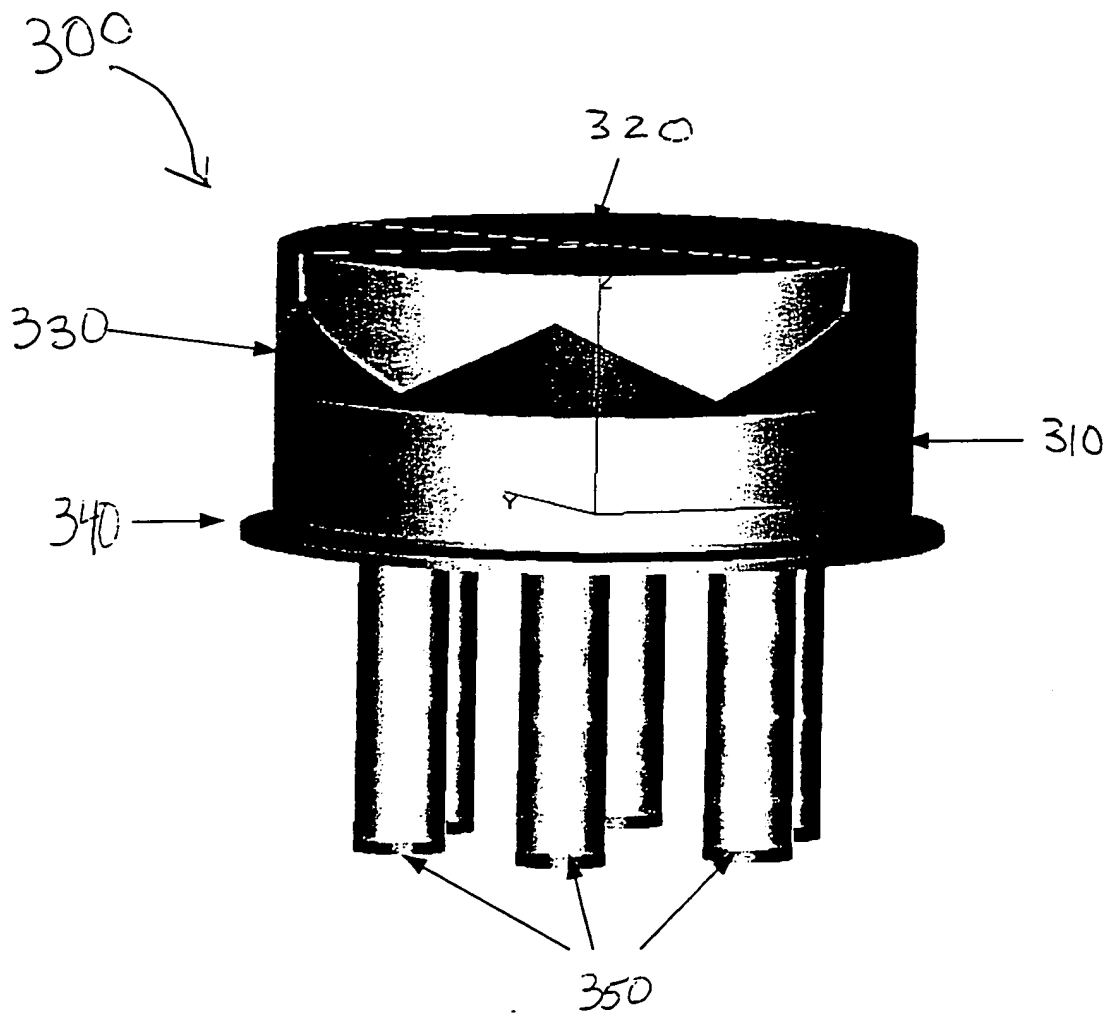


Fig. 10B

AU

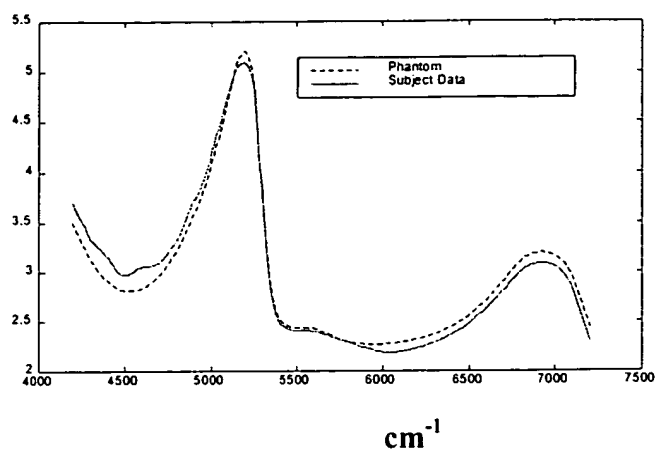


FIG. 11

4000 4500 5000 5500 6000 6500 7000 7500

FIG. 12

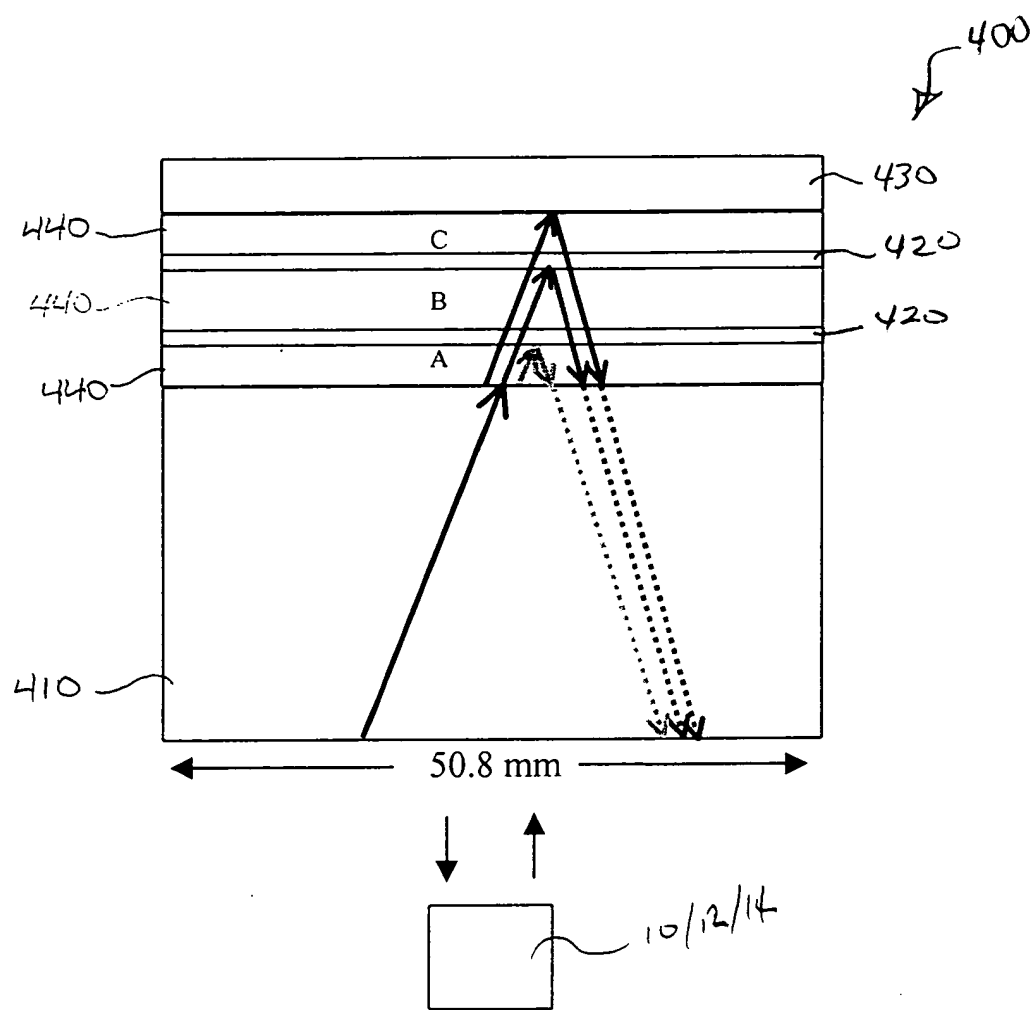


FIG. 12

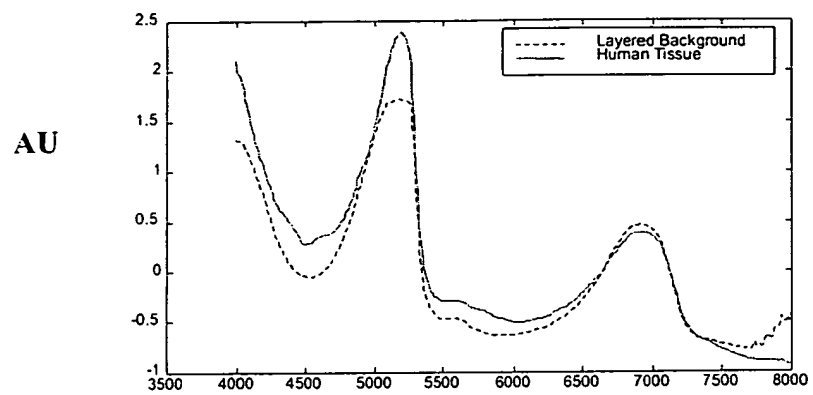


FIG. 13

09433600-0440-0000-0000-0000-0000

/

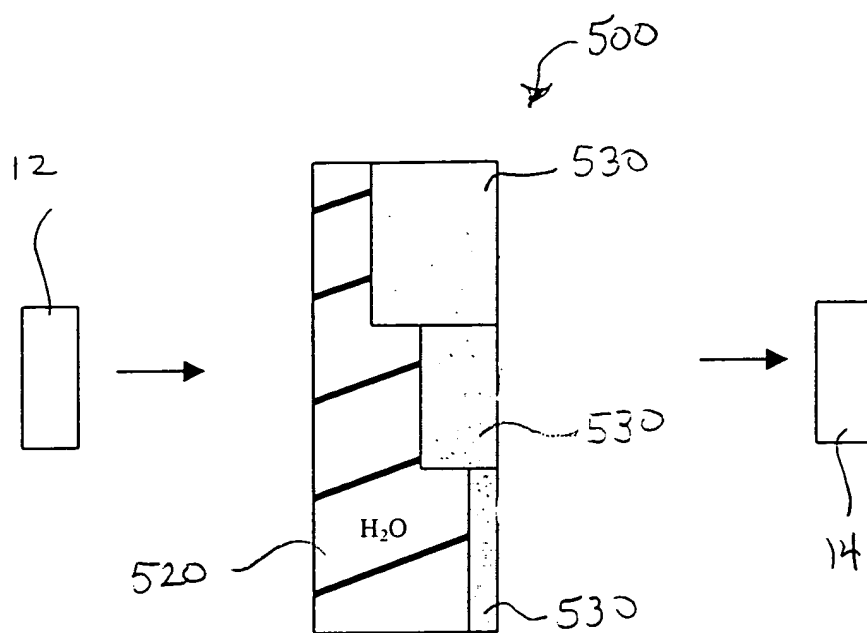


FIG. 14

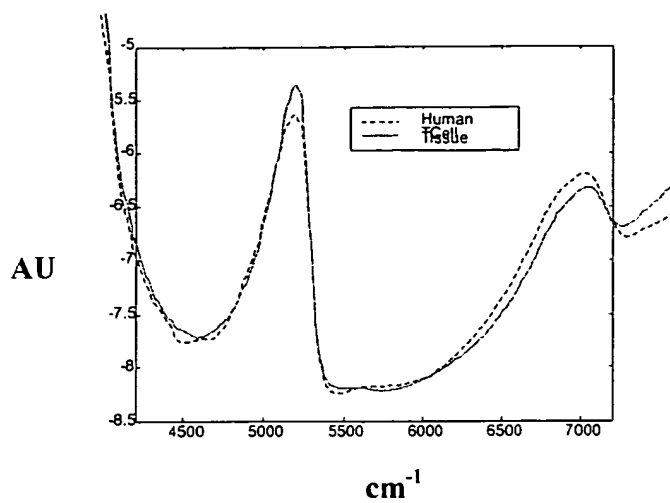


FIG. 15

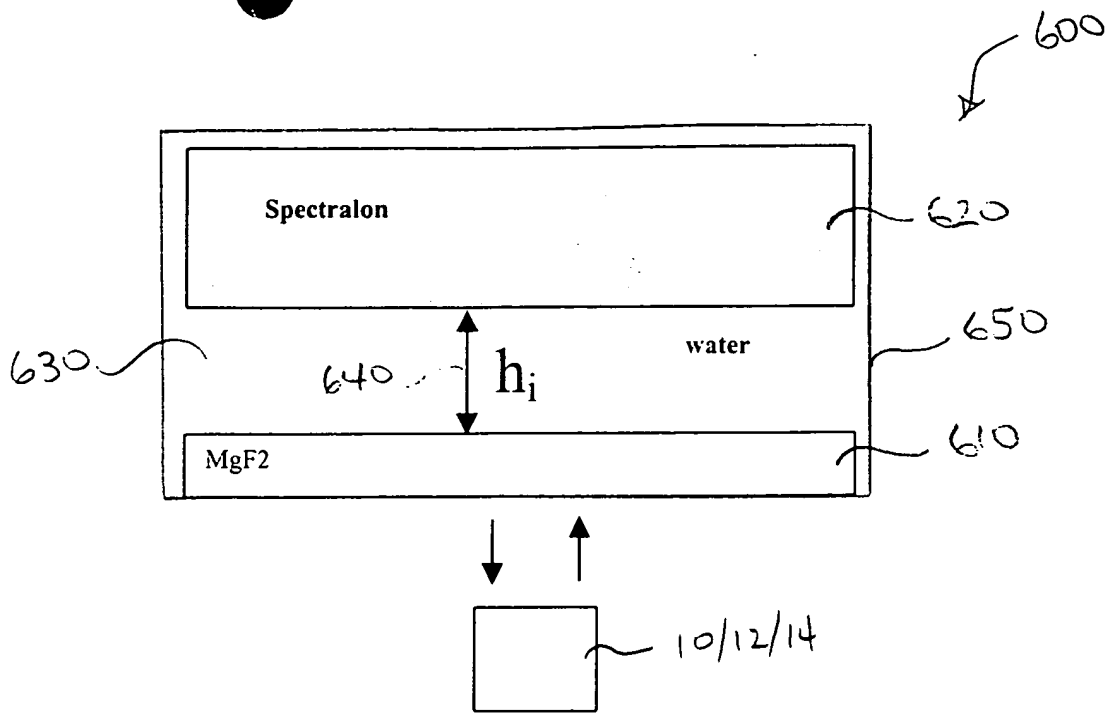


FIG. 16

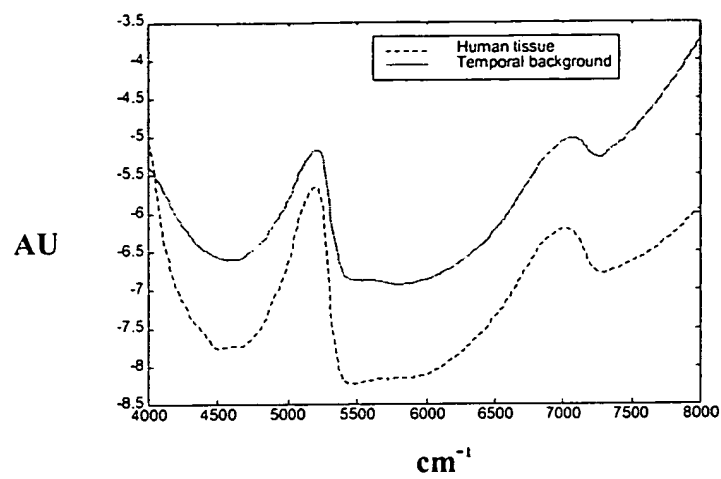


FIG. 17

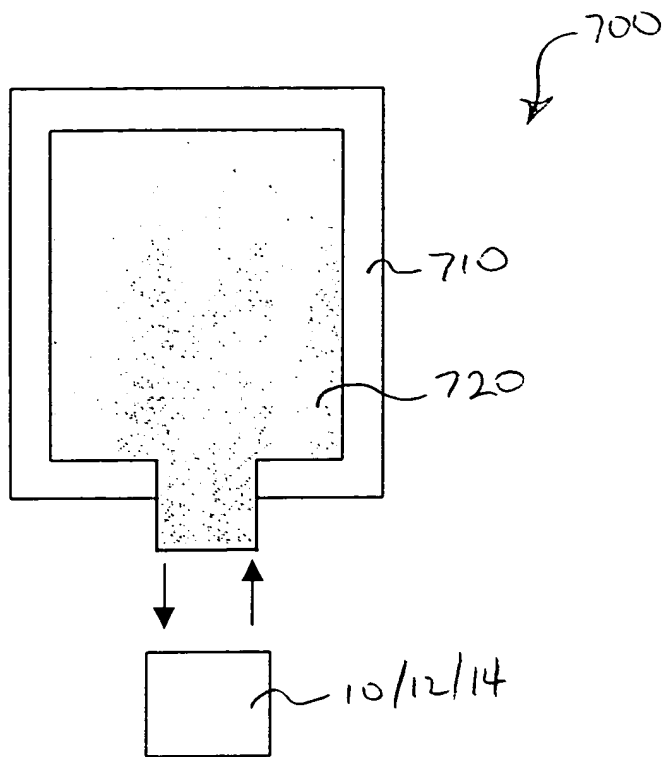


FIG. 18

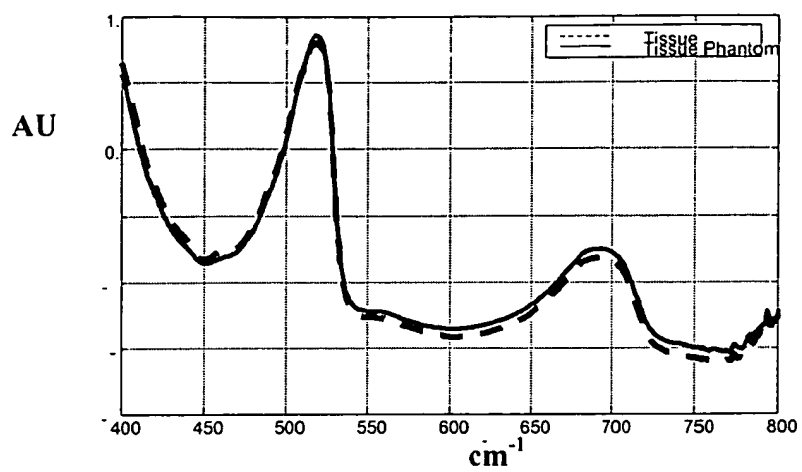


FIG. 19

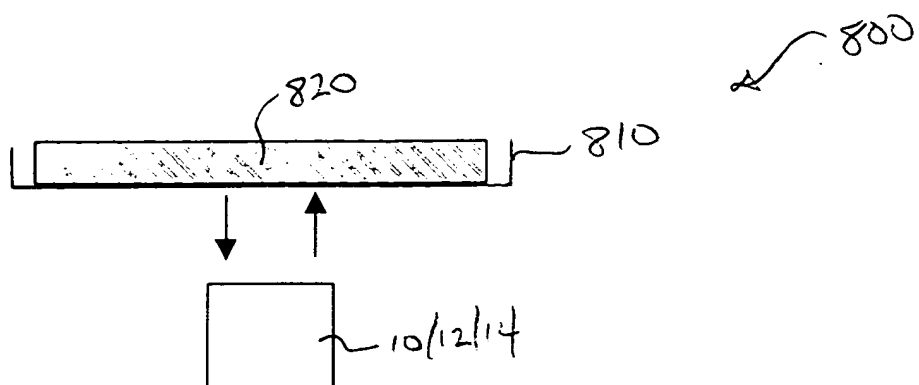


FIG. 20

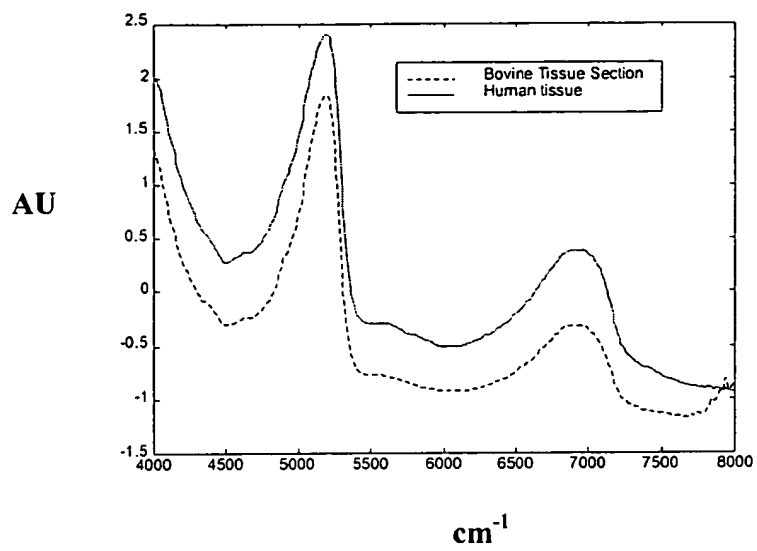


FIG. 21